

FIG. IA




FIG. IB

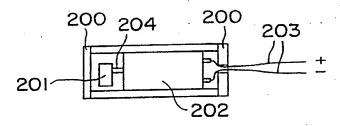



FIG. 2A




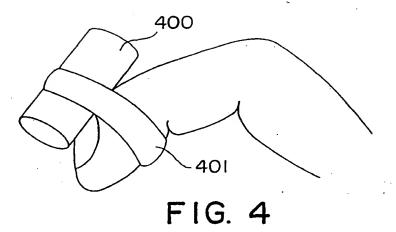


FIG. 3



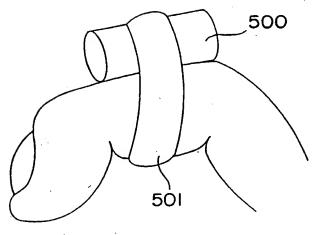


FIG. 5

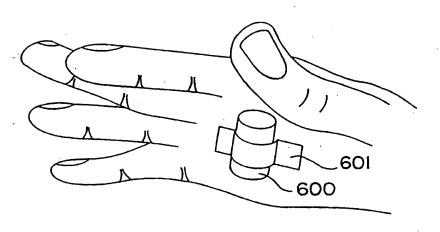
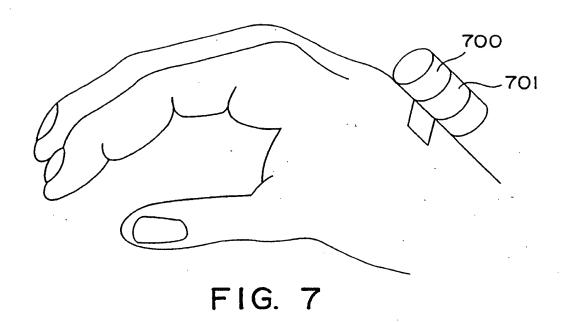
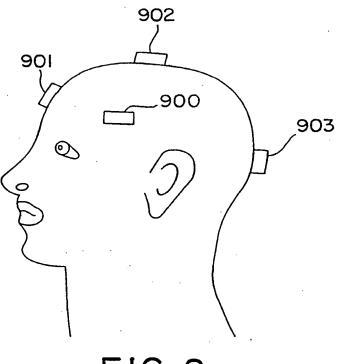


FIG. 6










FIG. 8

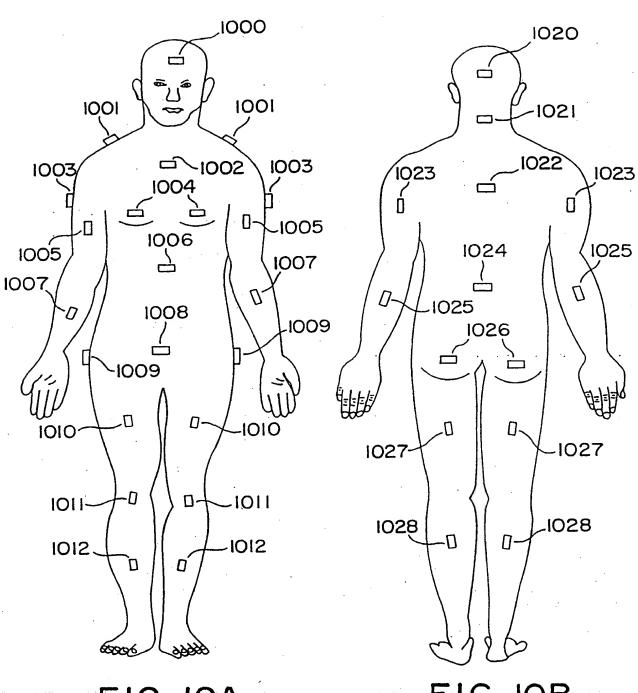
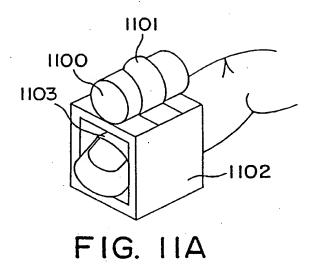




FIG. IOA

FIG. IOB












FIG. 12B



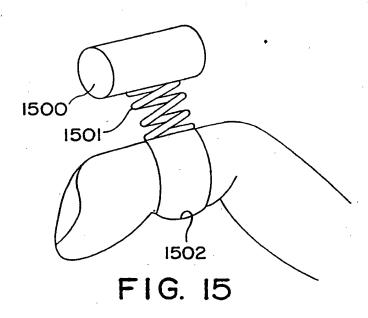
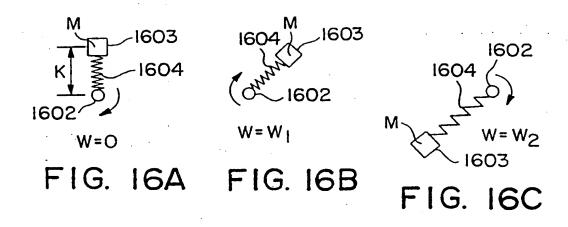


FIG. 13







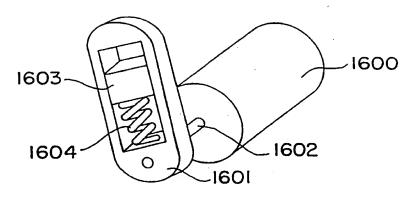
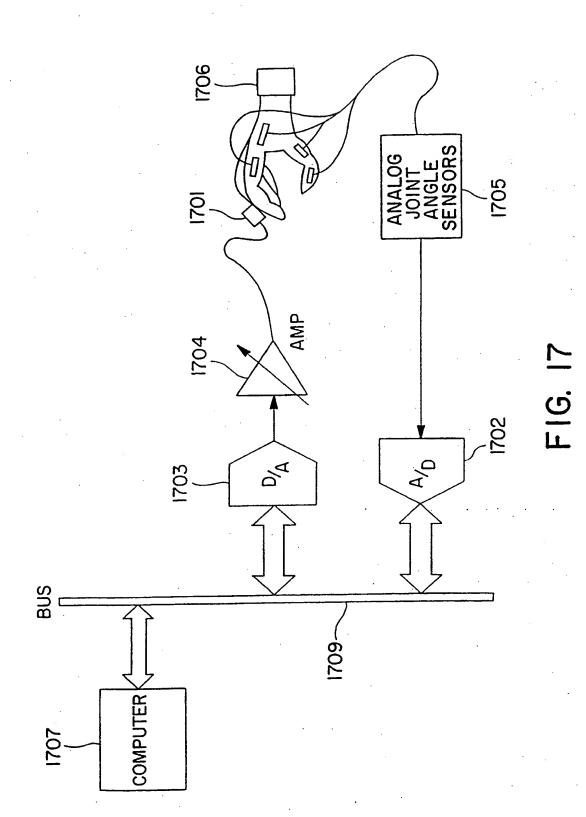
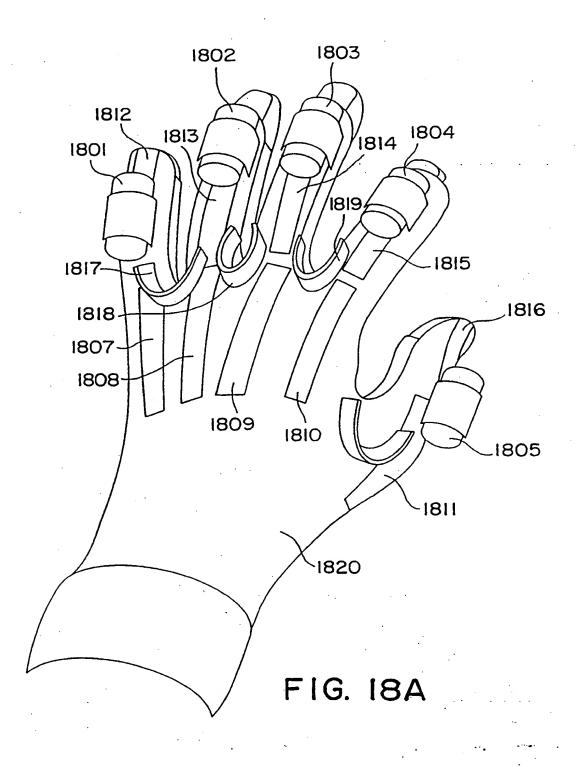
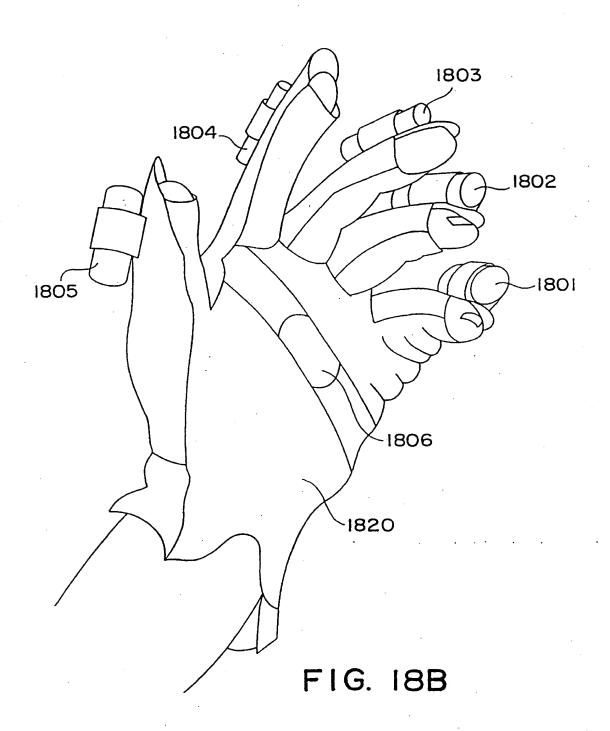
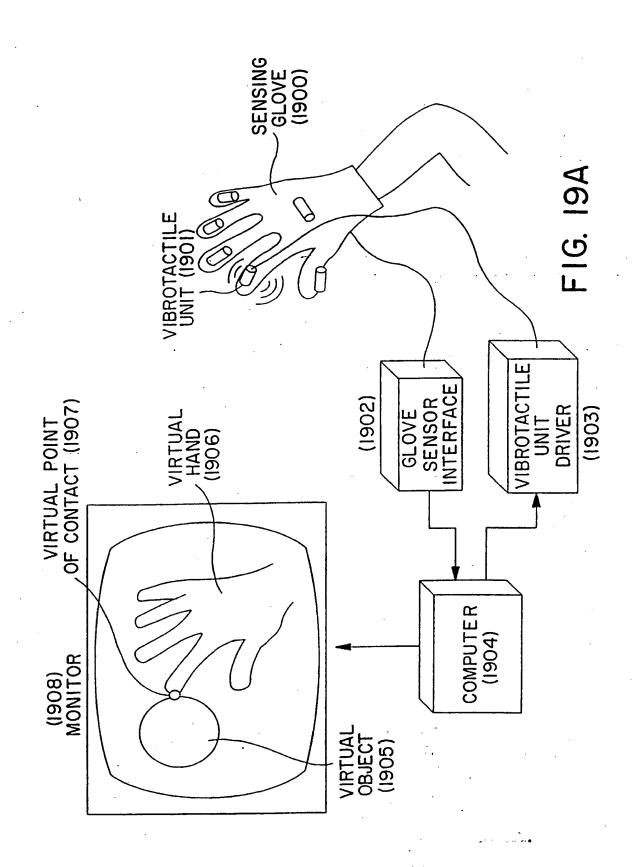



FIG. 16D












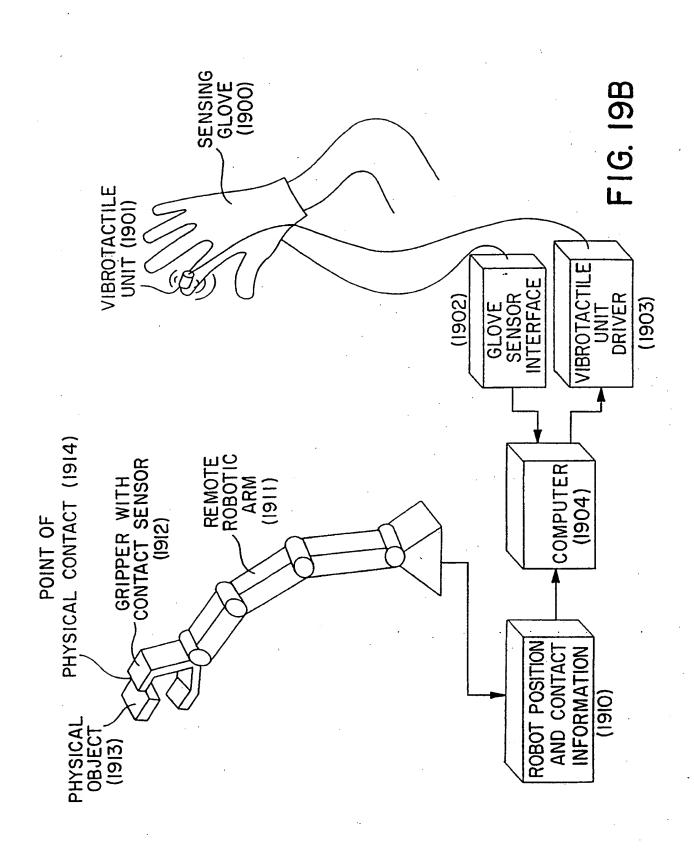

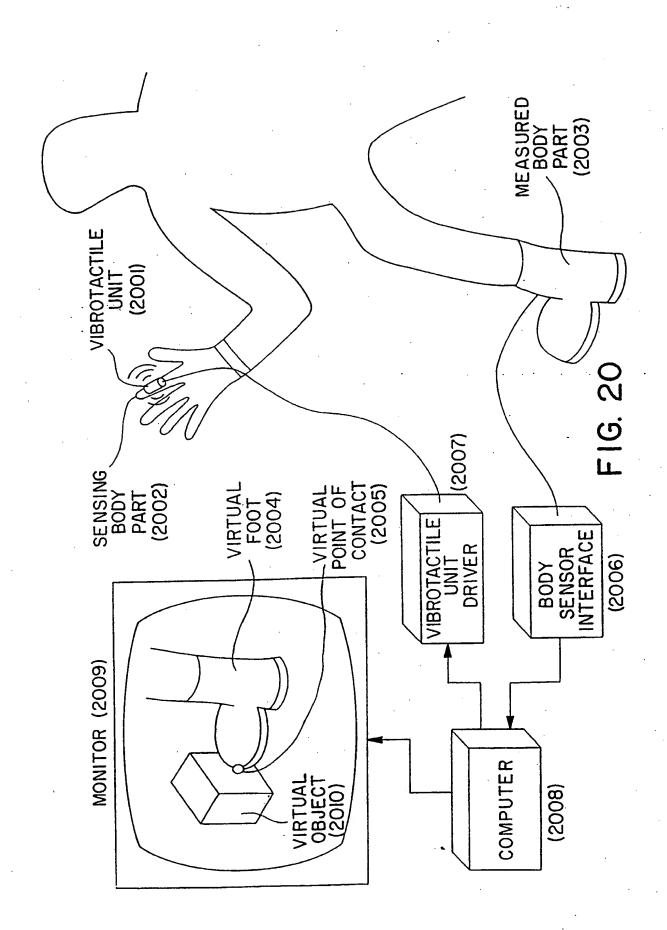

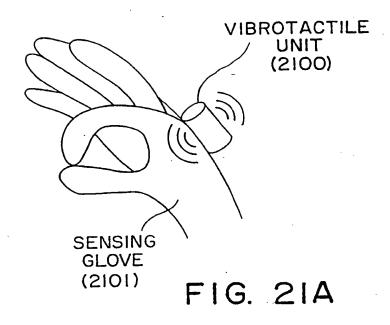

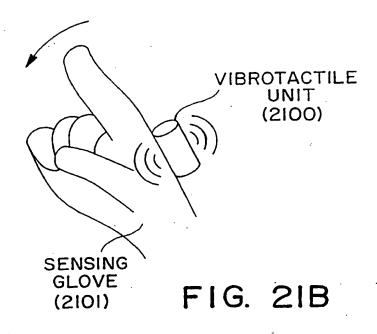

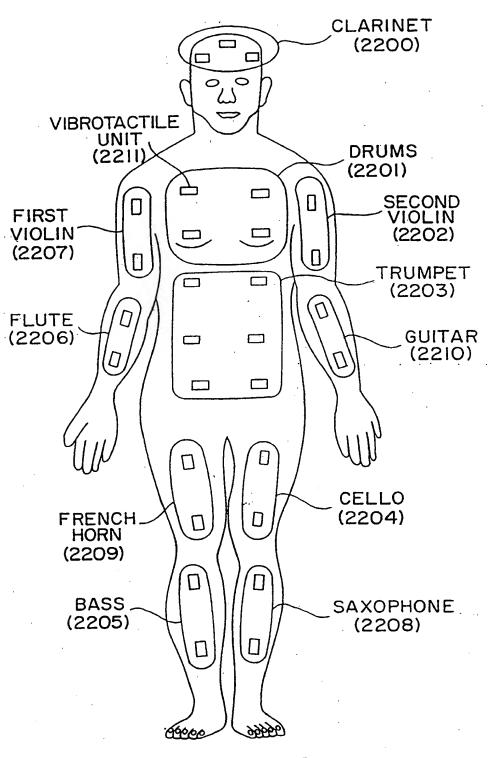
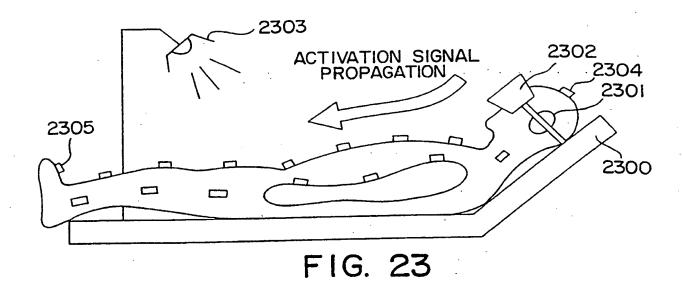
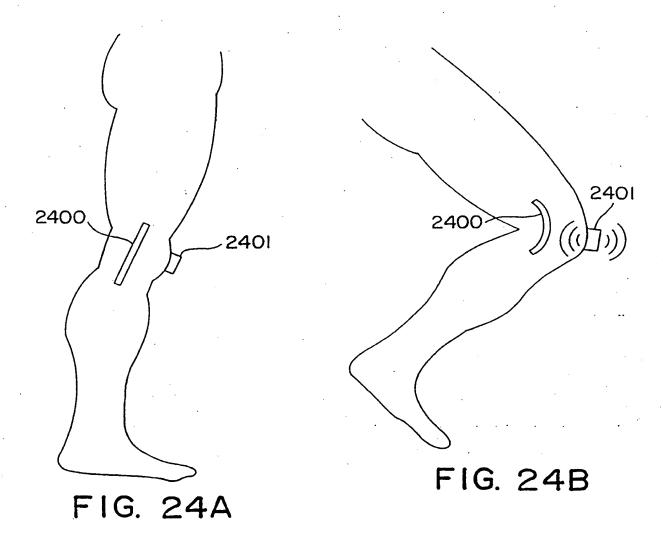
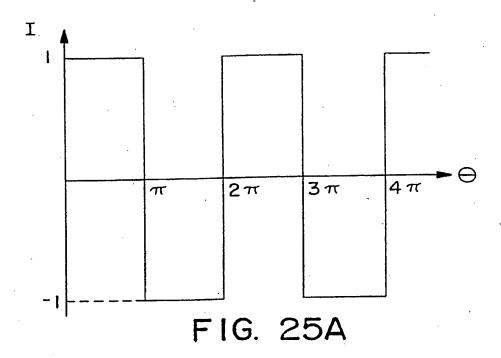


FIG. 22







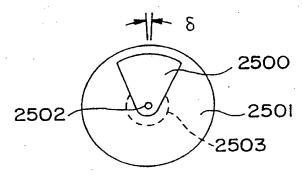
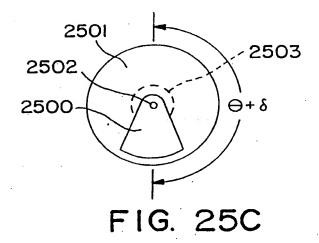


FIG. 25B



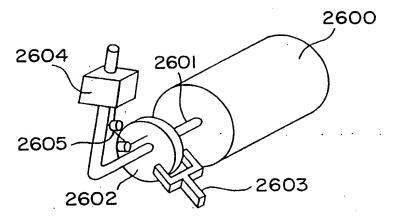


FIG. 26A




FIG. 26B

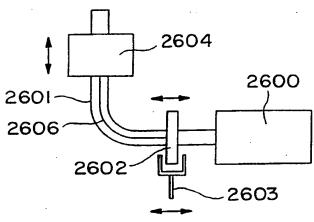


FIG. 26C

